

botiss**CARE**
empower **prevention**



QUICKGUIDE

botiss**CARE Cube Reader**

botiss**CARE Rapi-D™**

STEP-BY-STEP

test.
analyze.
prevent.





botiss**CARE Cube Reader**



botiss**CARE Rapi-D™**

only **15**
minutes

CONTENT



Sample container



Capillary



Lancet



Test cassette



RFID card



botiss**CARE**
Cube Reader



Batteries



Adaptor

not included



Timer

TEST



01

Use the lancet to prick a finger and draw blood. Wipe away the first droplet of blood.



02

Gently touch the tip of the capillary to the blood droplet.



Important

Be aware that the capillary must be **completely filled**.



03

Fully insert the capillary into the sample container and push firmly to close with a tight fit.



04




Shake **3-4 times** to **extract all of the blood** from the capillary and mix the solution.



05

Remove the cap.

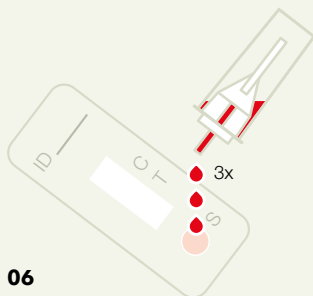

06


Gently squeeze **3 drops** into the sample well (S) of the test cassette.



07


Wait for **15 minutes**.
A shorter or longer waiting time **falsifies the test result**.
Two lines must be shown.





08

Place the adaptor on top of the test device in the **correct orientation** shown on the adaptor.



09

Place the Cube Reader in the **correct orientation** in the **correct orientation** shown on the adaptor.



10

Turn on the Cube Reader by pressing the black button.

If the Cube Reader does not turn on again straight after a test has been performed, press the button firmly and keep pressing until the Cube Reader turns back on.



11

After the first beep the last stored measured value is displayed. Press the black button.



12

After the beep **ON** is displayed.




13

Press the
button again.



14

The display will
show **RFID**.



15

Place the RFID Card provided
with the test kit on top.




16

After the beep **TEST**
is displayed. Press
the black button again.



17


The Cube Reader
displays **RUN**.

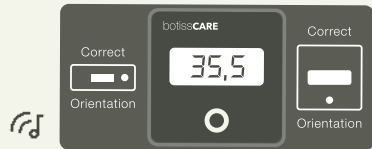

18

The vitamin D concentration is
displayed in **ng/ml**. The test
sequence is completed after
the last beep. After 50 sec.
the Cube Reader switches off
automatically.

Vitamin D level, 25-OH-D, **ng/ml** The test result is displayed in **ng/ml**

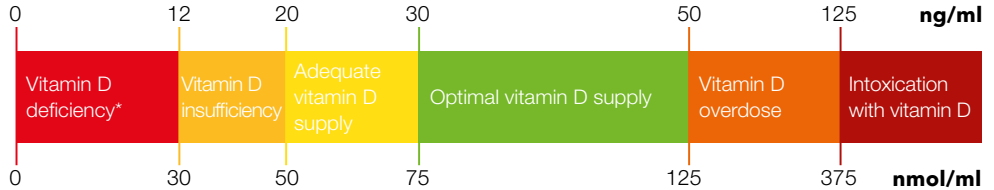

*In case of vitamin D levels below than 12 ng/ml, please consult a general physician for a proper vitamin D therapy.

Overview of vitamin D status derived from the various recommendations.
(From consilium theme booklet vitamin D)¹

Innovation. **360° Regeneration.** Aesthetics.

botiss stands for evidence-based know-how in bone and soft tissue regeneration. With innovative products, we are continuously developing our holistic 360° system together with international experts. Patient safety, treatment comfort, reliable and predictable treatment results are our first priority.

Driving dental **innovation.**



botiss biomaterials GmbH
Hauptstraße 28 · 15806 Zossen
botiss.com

¹National Institute of Health, USA